



5790A

Automated AC Measurement Standard

Technical Data



FLUKE 5790A AC MEASUREMENT STANDARD

2.1000456 V

10.000 KHZ

INPUT 1
1000V RMS MAX



INPUT 2
1000V RMS MAX

SHELL FLOATING
10V PEAK MAX

WIDEBAND
7V RMS MAX

SHUNT
3V RMS MAX

HI

LO

INPUT1

INPUT2

WBND

2.2 mV

22 mV

220 mV

7 mV

70 mV

700 mV

RESET

Accuracy that's easy to use

The 5790A is a complete automated ac measurement standard designed for the most demanding calibration applications. It combines the accuracy you would expect from a thermal transfer standard with the ease of use of a digital multimeter. Absolute ac voltage measurement uncertainties are as low as ± 24 ppm (one year, $23^{\circ}\text{C} \pm 5^{\circ}\text{C}$). The 5790A is designed to meet the complete ac voltage and wideband verification requirements of the Fluke 5700A, 5500A, and 5100 Series and other calibrators, amplifiers like the 5725A and 5205A, and transfer standards and ac voltmeters.

The 5790A covers an alternating voltage range of $700 \mu\text{V}$ to 1000V , and a frequency range of 10 Hz to 1 MHz . A wideband voltage option extends frequency range to 30 MHz to meet the calibration requirements of the Fluke 5700A, and 5100 Series calibrators.

The 5790A is also compatible with Fluke A40 and A40A Current Shunts, which permit you to make ac/dc current transfer measurements up to 20A .

The 5790A may be used alone or as a transfer standard with an external dc source. In either case the normally tedious switching and calculations are performed automatically by the 5790A, and the resulting ac/dc difference is displayed directly on the easy-to-read vacuum fluorescent display.

Precision you can depend on

The 5790A is based on the patented Fluke Solid-State Thermal RMS Sensor, which has been proven since 1979 in a variety of Fluke products like the 792A AC/DC Transfer Standard. The Fluke RMS Sensor is a *true* thermal converter, not an electronic converter that calculates the RMS value. Because its output voltage is 2V rather than the 7 to 10 mV of traditional thermocouples, the RMS sensor exhibits excellent signal-to-noise characteristics and minimal reversal errors. With a higher output voltage, more accurate measurements can be made. And because of its small size, the RMS sensor stabilizes quickly and operates over a wide temperature range.

The 5790A also features hermetically sealed thin-film resistor networks to minimize ac measurement errors and enhance temperature coefficient.

The RMS sensor and thin-film resistor networks are designed by Fluke to be rugged and reliable. Each is built to exacting standards by the Fluke Microelectronics Operation to maintain quality and consistency part after part.


Versatility that keeps you productive

When you first power up the 5790A, diagnostics verify the instrument's integrity.

The variety of input connections allows you to use the one that best suits your application. There are four sets of input terminals on the 5790A, two Type-N connectors and two sets of five-way binding posts. One Type-N and one set of binding posts are dedicated to the ac measurement and transfer modes. AC or dc voltages may be applied to either input connection over the 5790A's full range, allowing you to perform automated ac/dc transfer measurements. The 5790A determines automatically whether the applied voltage is ac or dc.



The 5790A is compatible with Fluke A40 and A40A Current Shunts to permit measurements to 20A .

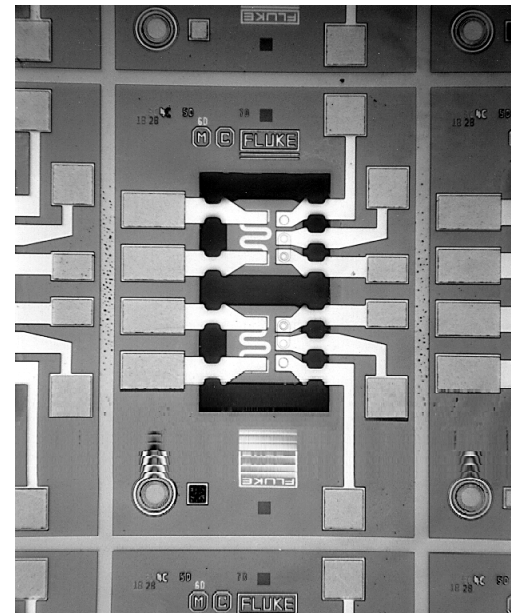

The patented Fluke Solid-State RMS Sensor provides the 5790A with exceptional accuracy and stability, and fast settling time.

1 Low-loss Type-N connector for the best performance above 20 kHz or as the input for the ac voltage when automated ac/dc difference measurements are made. These inputs may be used over the 5790A's full voltage range of 700 μ V to 1000V.

2 Low thermal emf tellurium copper alloy binding posts for general measurements and as the dc voltage input when automated ac/dc difference measurements are made.

3 These binding posts permit the use of A40 shunts to make ac/dc current difference measurements.


4 Low-loss Type-N connector for making wideband voltage measurements from 10 Hz to 30 MHz (Option -03).

5 These keys allow you to select one of the four inputs. An illuminated LED indicates which input has been selected.

6 These keys are used to manually select the desired voltage range for the present measurement.

7 $\uparrow\downarrow$ keys allow you to select one range higher or lower.

8 These "soft" keys allow you to work with the menus displayed on the control screen above.

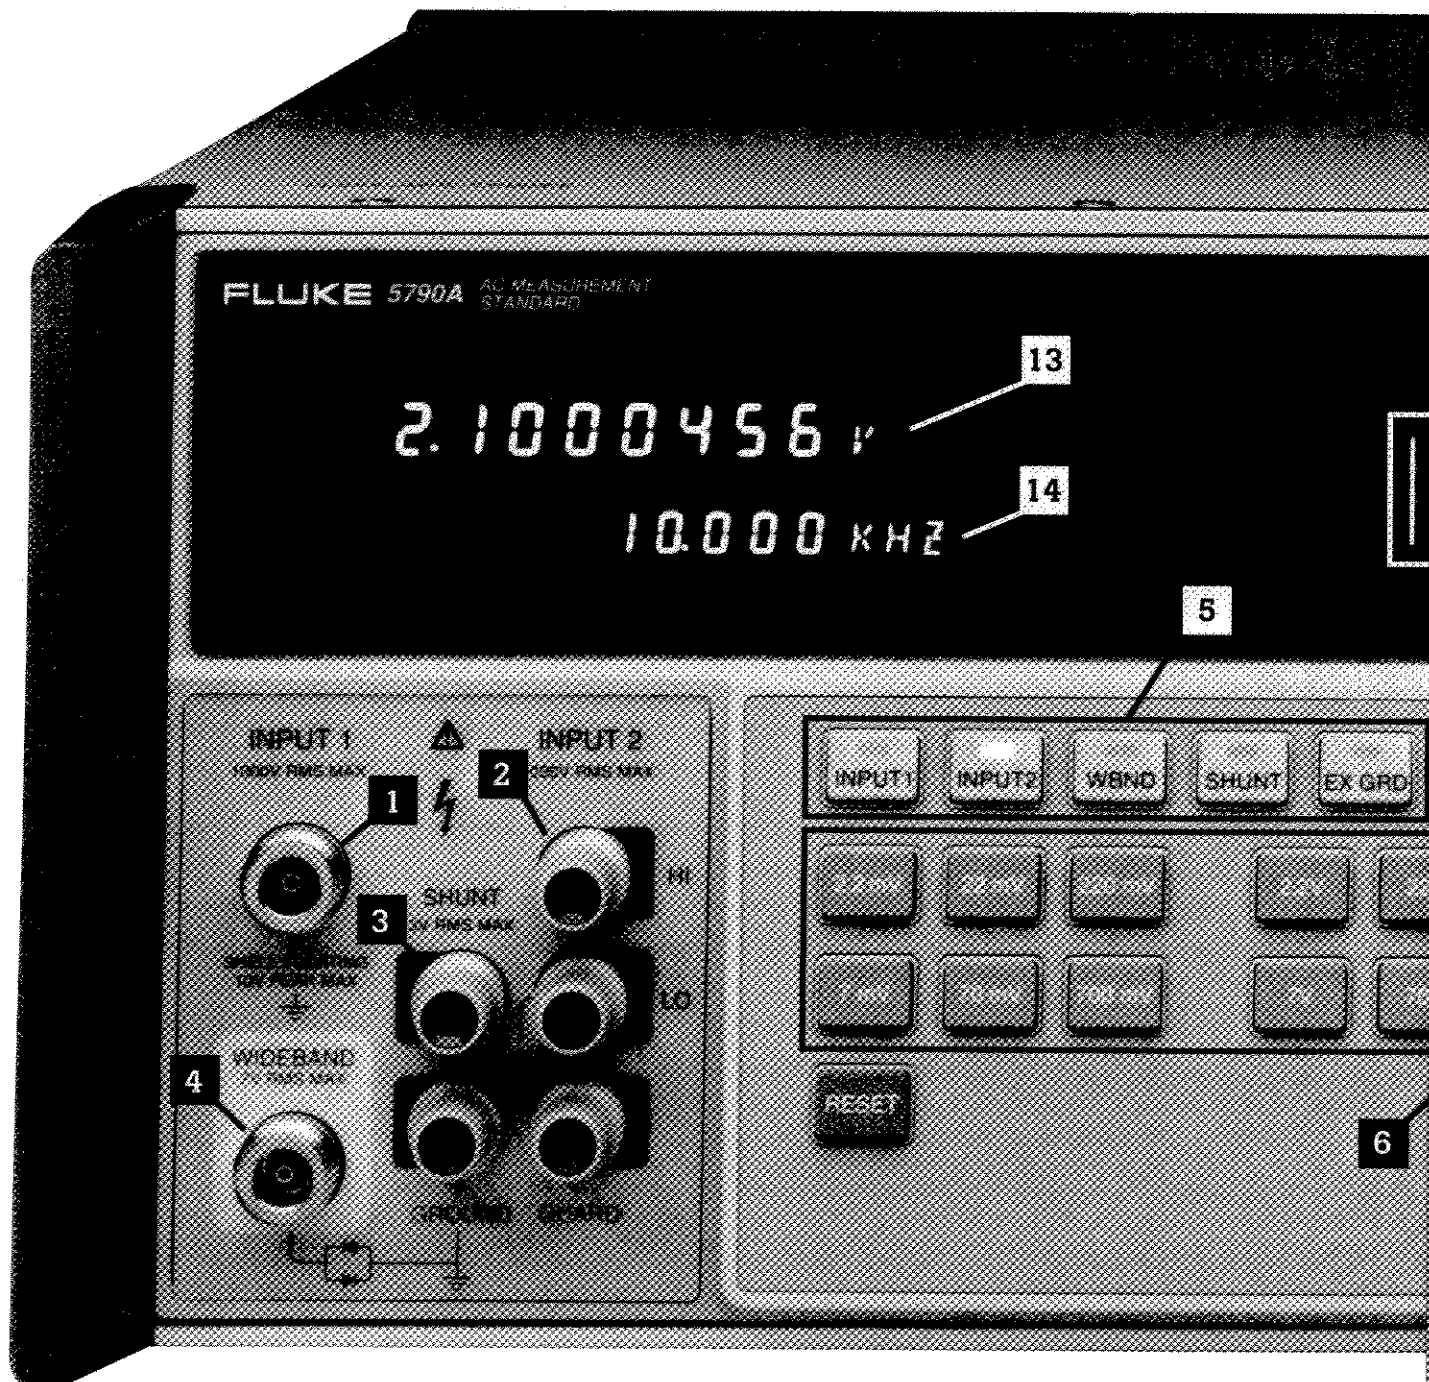

9 Allows you to display the reference for an ac/dc transfer measurement.

10 Displays the instrument's utility menu. Use the "soft" keys to select the desired utility, including remote port parameters, calibration, diagnostics and general instrument set-up.

11 Displays the total uncertainty for the most recent measurement.

12 Choose between continuous measurements or single measurement.

13 The input voltage is always displayed on the upper portion of the measurement display.

14 The frequency of the applied ac voltage is displayed on the lower portion of the measurement display.

15 The control display shows information on the status of the instrument during measurements or maintenance and indicates the function of the "soft" keys directly below the display.



The second Type-N input connection supports the optional wideband mode, and the second set of binding posts are designed for Fluke A40 Series current shunts.

The input connection is selected with the touch of a key on the 5790A front panel. An LED indicates which selection is active.

Whether you are using the 5790A as a voltmeter or a transfer standard, input voltage and frequency are always indicated on the measurement display. In the transfer mode, the ac/dc or ac/ac difference is always indicated on the control display in ppm, %, volts or ratio.

The 5790A is a fully autoranging instrument and selects the best voltage range for the measurement you are making. You may also select and lock in ranges manually. Robust 1200V input protection is active on all voltage ranges.

Using the trigger keys, the 5790A can switch from continuous to single measurements of the input voltage, making it easy to take sample readings at predetermined intervals.

When using the 5790A in transfer mode, the reference voltage is stored automatically, and all ac/dc or ac/ac difference measurements are made relative to it. At any time, you can view the reference by pressing the VIEW REF key. You may also store the average of two voltages as a reference to eliminate dc reversal errors, for example.

The intuitive front panel layout of the 5790A makes manual operation fast and simple. Keys and selections are logically arranged and labelled. And messages and menus are displayed clearly on the 5790A's bright, vacuum fluorescent display.



The 5790A is designed to meet the ac verification requirements of the Fluke 5700A Calibrator. Automation using MET/CAL Calibration Software is fast and easy.

The 5790A is at home in automated systems as well. IEEE-488 and RS-232 interfaces are included and all functions of the instruments can be controlled by a variety of host computers, including PCs. The 5790A can be integrated into automated systems operating under MET/CAL™ Calibration Software.

Designed with your support requirements in mind

The 5790A provides a self-contained calibration procedure designed to simplify periodic performance verification. The operator is prompted on what actions to take. To minimize the equipment required, the 5790A is designed to be supported by the Fluke 792A AC/DC Transfer Standard.



Traceability to national standards for the 5790A is supported through the Fluke 792A.

Performance specifications

To simplify evaluation of how the 5790A covers your calibration workload, use the Absolute Uncertainty Specifications.

Absolute Uncertainties include stability, temperature coefficient, linearity and traceability to external standards. *You do not need to add any-*

thing to determine the ratios between 5790A uncertainties and the uncertainties of your calibration workload when used within $\pm 5^{\circ}\text{C}$ of calibration temperature.

Relative Uncertainty specifications are provided so that absolute uncertainties may be

calculated when equipment or traceability differ from what is specified in the calibration section of the 5790A manual.

Secondary Performance and Operating Characteristics are provided for special calibration requirements such as stability or operation at temperature extremes.

Absolute Uncertainty Specifications

$\pm 5^{\circ}\text{C}$ of Calibration Temperature

Voltage Range	Frequency Range	Absolute Uncertainty			
		AC/DC Transfer Mode	Measurement Mode		
		$\pm\text{PPM}$	$\pm(\text{PPM of Reading} + \mu\text{V})$		
		2 Years	90 Days	1 Year	2 Years
2.2 mV	10 Hz - 20 Hz		1700+1.3	1700+1.3	1700+1.3
	20 Hz - 40 Hz		740+1.3	740+1.3	740+1.3
	40 Hz - 20 kHz		420+1.3	420+1.3	420+1.3
	20 kHz - 50 kHz		810+2.0	810+2.0	820+2.0
	50 kHz - 100 kHz		1200+2.5	1200+2.5	1200+2.5
	100 kHz - 300 kHz		2300+4.0	2300+4.0	2300+4.0
	300 kHz - 500 kHz 500 kHz - 1 MHz		2400+6.0 3200+6.0	2400+8.0 3500+8.0	2600+8.0 5000+8.0
7 mV	10 Hz - 20 Hz		850+1.3	850+1.3	850+1.3
	20 Hz - 40 Hz		370+1.3	370+1.3	370+1.3
	40 Hz - 20 kHz		210+1.3	210+1.3	210+1.3
	20 kHz - 50 kHz		400+2.0	400+2.0	410+2.0
	50 kHz - 100 kHz		600+2.5	600+2.5	610+2.5
	100 kHz - 300 kHz		1200+4.0	1200+4.0	1200+4.0
	300 kHz - 500 kHz 500 kHz - 1 MHz		1300+6.0 2000+6.0	1300+8.0 2300+8.0	1400+8.0 3600+8.0
22 mV	10 Hz - 20 Hz		290+1.3	290+1.3	290+1.3
	20 Hz - 40 Hz		180+1.3	190+1.3	190+1.3
	40 Hz - 20 kHz		110+1.3	110+1.3	110+1.3
	20 kHz - 50 kHz		210+2.0	210+2.0	210+2.0
	50 kHz - 100 kHz		310+2.5	310+2.5	310+2.5
	100 kHz - 300 kHz		810+4.0	810+4.0	820+4.0
	300 kHz - 500 kHz 500 kHz - 1 MHz		860+6.0 1400+6.0	890+8.0 1700+8.0	1000+8.0 2600+8.0
70 mV	10 Hz - 20 Hz		240+1.5	240+1.5	240+1.5
	20 Hz - 40 Hz		120+1.5	120+1.5	130+1.5
	40 Hz - 20 kHz		64+1.5	65+1.5	69+1.5
	20 kHz - 50 kHz		120+2.0	130+2.0	130+2.0
	50 kHz - 100 kHz		260+2.5	260+2.5	260+2.5
	100 kHz - 300 kHz		510+4.0	510+4.0	530+4.0
	300 kHz - 500 kHz 500 kHz - 1 MHz		660+6.0 1100+6.0	670+8.0 1100+8.0	680+8.0 1300+8.0
220 mV	10 Hz - 20 Hz	210	210+1.5	210+1.5	210+1.5
	20 Hz - 40 Hz	82	84+1.5	85+1.5	87+1.5
	40 Hz - 20 kHz	34	37+1.5	38+1.5	43+1.5
	20 kHz - 50 kHz	67	69+2.0	69+2.0	73+2.0
	50 kHz - 100 kHz		160+2.5	160+2.5	160+2.5
	100 kHz - 300 kHz		240+4.0	250+4.0	280+4.0
	300 kHz - 500 kHz 500 kHz - 1 MHz		360+6.0 940+6.0	380+8.0 1000+8.0	400+8.0 1200+8.0
700 mV	10 Hz - 20 Hz	210	210+1.5	210+1.5	210+1.5
	20 Hz - 40 Hz	73	75+1.5	76+1.5	78+1.5
	40 Hz - 20 kHz	27	31+1.5	33+1.5	38+1.5
	20 kHz - 50 kHz	47	50+2.0	51+2.0	56+2.0
	50 kHz - 100 kHz		79+2.5	79+2.5	84+2.5
	100 kHz - 300 kHz		160+4.0	180+4.0	210+4.0
	300 kHz - 500 kHz 500 kHz - 1 MHz		300+6.0 900+6.0	300+8.0 960+8.0	340+8.0 1200+8.0
$\pm(\text{PPM of Reading})$					
2.2V	10 Hz - 20 Hz	200	200	200	200
	20 Hz - 40 Hz	63	65	66	69
	40 Hz - 20 kHz	18	22	24	29
	20 kHz - 50 kHz	43	45	46	52
	50 kHz - 100 kHz		70	71	76
	100 kHz - 300 kHz		150	160	200
	300 kHz - 500 kHz 500 kHz - 1 MHz		250 840	260 900	310 1200

Absolute Uncertainty Specifications (continued)

±5°C of Calibration Temperature

Voltage Range	Frequency Range	Absolute Uncertainty			
		AC/DC Transfer Mode	Measurement Mode		
		±PPM	±(PPM of Reading)		
		2 Years	90 Days	1 Year	2 Years
7V	10 Hz - 20 Hz	200	200	200	200
	20 Hz - 40 Hz	63	66	67	70
	40 Hz - 20 kHz	18	22	24	29
	20 kHz - 50 kHz	44	46	48	53
	50 kHz - 100 kHz		80	81	88
	100 kHz - 300 kHz		180	190	220
	300 kHz - 500 kHz		380	400	470
	500 kHz - 1 MHz		1100	1200	1500
22V	10 Hz - 20 Hz	200	200	200	200
	20 Hz - 40 Hz	63	66	67	70
	40 Hz - 20 kHz	21	25	27	31
	20 kHz - 50 kHz	44	46	48	53
	50 kHz - 100 kHz		80	81	85
	100 kHz - 300 kHz		180	190	220
	300 kHz - 500 kHz		380	400	470
	500 kHz - 1 MHz		1100	1200	1500
70V	10 Hz - 20 Hz	200	200	200	200
	20 Hz - 40 Hz	63	67	68	72
	40 Hz - 20 kHz	25	30	32	39
	20 kHz - 50 kHz	55	56	57	63
	50 kHz - 100 kHz		91	94	110
	100 kHz - 300 kHz		190	200	220
	300 kHz - 500 kHz		400	410	510
	500 kHz - 1 MHz		1100	1200	1500
220V	10 Hz - 20 Hz	200	200	200	200
	20 Hz - 40 Hz	63	67	68	72
	40 Hz - 20 kHz	23	29	31	38
	20 kHz - 50 kHz	63	67	69	77
	50 kHz - 100 kHz		96	98	110
	100 kHz - 300 kHz		210	210	260
	300 kHz - 500 kHz		440	500	700
700V	10 Hz - 20 Hz	200	200	200	200
	20 Hz - 40 Hz	92	96	99	110
	40 Hz - 20 kHz	36	39	41	47
	20 kHz - 50 kHz		120	130	150
	50 kHz - 100 kHz		400	500	850
1000V	10 Hz - 20 Hz	200	200	200	200
	20 Hz - 40 Hz	92	96	99	110
	40 Hz - 20 kHz	33	37	38	44
	20 kHz - 50 kHz		120	130	150
	50 kHz - 100 kHz		400	500	850

Relative Uncertainty Specifications

±5°C of Calibration Temperature

Voltage Range	Frequency Range	Relative Uncertainty			
		AC/DC Transfer Mode	Measurement Mode		
		±PPM	±(PPM of Reading + μV)		
		2 Years	90 Days	1 Year	2 Years
2.2 mV	10 Hz - 20 Hz		100 + 1.3	110 + 1.3	110 + 1.3
	20 Hz - 40 Hz		54 + 1.3	64 + 1.3	68 + 1.3
	40 Hz - 20 kHz		44 + 1.3	57 + 1.3	61 + 1.3
	20 kHz - 50 kHz		57 + 2.0	67 + 2.0	110 + 2.0
	50 kHz - 100 kHz		79 + 2.5	86 + 2.5	120 + 2.5
	100 kHz - 300 kHz		190 + 4.0	230 + 4.0	390 + 4.0
	300 kHz - 500 kHz		590 + 6.0	720 + 8.0	1200 + 8.0
	500 kHz - 1 MHz		2200 + 6.0	2600 + 8.0	4400 + 8.0
7 mV	10 Hz - 20 Hz		80 + 1.3	83 + 1.3	86 + 1.3
	20 Hz - 40 Hz		33 + 1.3	39 + 1.3	45 + 1.3
	40 Hz - 20 kHz		29 + 1.3	36 + 1.3	42 + 1.3
	20 kHz - 50 kHz		40 + 2.0	44 + 2.0	63 + 2.0
	50 kHz - 100 kHz		53 + 2.5	57 + 2.5	72 + 2.5
	100 kHz - 300 kHz		110 + 4.0	130 + 4.0	210 + 4.0
	300 kHz - 500 kHz		370 + 6.0	450 + 8.0	740 + 8.0
	500 kHz - 1 MHz		1600 + 6.0	2000 + 8.0	3400 + 8.0

Relative Uncertainty Specifications (continued)

±5°C of Calibration Temperature

Voltage Range	Frequency Range	Relative Uncertainty			
		AC/DC Transfer Mode	Measurement Mode		
		±PPM	±(PPM of Reading + μV)		
		2 Years	90 Days	1 Year	2 Years
22 mV	10 Hz - 20 Hz		69 + 1.3	72 + 1.3	75 + 1.3
	20 Hz - 40 Hz		34 + 1.3	40 + 1.3	46 + 1.3
	40 Hz - 20 kHz		30 + 1.3	36 + 1.3	43 + 1.3
	20 kHz - 50 kHz		40 + 2.0	45 + 2.0	64 + 2.0
	50 kHz - 100 kHz		53 + 2.5	57 + 2.5	73 + 2.5
	100 kHz - 300 kHz		97 + 4.0	110 + 4.0	160 + 4.0
	300 kHz - 500 kHz		310 + 6.0	380 + 8.0	610 + 8.0
	500 kHz - 1 MHz		1200 + 6.0	1500 + 8.0	2500 + 8.0
70 mV	10 Hz - 20 Hz		60 + 1.5	61 + 1.5	62 + 1.5
	20 Hz - 40 Hz		27 + 1.5	30 + 1.5	37 + 1.5
	40 Hz - 20 kHz		22 + 1.5	25 + 1.5	34 + 1.5
	20 kHz - 50 kHz		34 + 2.0	36 + 2.0	44 + 2.0
	50 kHz - 100 kHz		53 + 2.5	54 + 2.5	62 + 2.5
	100 kHz - 300 kHz		110 + 4.0	120 + 4.0	170 + 4.0
	300 kHz - 500 kHz		270 + 6.0	290 + 8.0	320 + 8.0
	500 kHz - 1 MHz		910 + 6.0	970 + 8.0	1200 + 8.0
220 mV	10 Hz - 20 Hz	55	60 + 1.5	61 + 1.5	62 + 1.5
	20 Hz - 40 Hz	20	27 + 1.5	29 + 1.5	35 + 1.5
	40 Hz - 20 kHz	17	22 + 1.5	24 + 1.5	31 + 1.5
	20 kHz - 50 kHz	17	22 + 2.0	24 + 2.0	33 + 2.0
	50 kHz - 100 kHz		51 + 2.5	52 + 2.5	59 + 2.5
	100 kHz - 300 kHz		100 + 4.0	120 + 4.0	170 + 4.0
	300 kHz - 500 kHz		260 + 6.0	290 + 8.0	310 + 8.0
	500 kHz - 1 MHz		890 + 6.0	950 + 8.0	1200 + 8.0
700 mV	10 Hz - 20 Hz	55	60 + 1.5	61 + 1.5	62 + 1.5
	20 Hz - 40 Hz	20	27 + 1.5	29 + 1.5	34 + 1.5
	40 Hz - 20 kHz	15	22 + 1.5	24 + 1.5	31 + 1.5
	20 kHz - 50 kHz	15	22 + 2.0	24 + 2.0	33 + 2.0
	50 kHz - 100 kHz		51 + 2.5	52 + 2.5	59 + 2.5
	100 kHz - 300 kHz		100 + 4.0	120 + 4.0	170 + 4.0
	300 kHz - 500 kHz		260 + 6.0	270 + 8.0	310 + 8.0
	500 kHz - 1 MHz		890 + 6.0	950 + 8.0	1200 + 8.0
±(PPM of Reading)					
2.2V	10 Hz - 20 Hz	55	60	61	62
	20 Hz - 40 Hz	19	26	28	34
	40 Hz - 20 kHz	15	20	22	27
	20 kHz - 50 kHz	15	21	23	33
	50 kHz - 100 kHz		49	50	57
	100 kHz - 300 kHz		92	110	160
	300 kHz - 500 kHz		220	230	280
	500 kHz - 1 MHz		830	890	1200
7V	10 Hz - 20 Hz	55	60	61	62
	20 Hz - 40 Hz	19	27	29	36
	40 Hz - 20 kHz	15	20	22	27
	20 kHz - 50 kHz	18	23	26	35
	50 kHz - 100 kHz		62	64	73
	100 kHz - 300 kHz		140	150	180
	300 kHz - 500 kHz		360	380	450
	500 kHz - 1 MHz		1100	1200	1500
22V	10 Hz - 20 Hz	55	60	61	62
	20 Hz - 40 Hz	19	28	30	37
	40 Hz - 20 kHz	15	20	22	27
	20 kHz - 50 kHz	18	23	26	35
	50 kHz - 100 kHz		62	64	69
	100 kHz - 300 kHz		140	150	180
	300 kHz - 500 kHz		360	380	450
	500 kHz - 1 MHz		1100	1200	1500
70V	10 Hz - 20 Hz	55	60	62	63
	20 Hz - 40 Hz	19	29	31	39
	40 Hz - 20 kHz	15	23	25	34
	20 kHz - 50 kHz	22	25	27	39
	50 kHz - 100 kHz		64	68	85
	100 kHz - 300 kHz		140	150	180
	300 kHz - 500 kHz		370	390	490
	500 kHz - 1 MHz		1100	1200	1500

Relative Uncertainty Specifications (continued)

±5°C of Calibration Temperature

Voltage Range	Frequency Range	Relative Uncertainty			
		AC/DC Transfer Mode	Measurement Mode		
		±PPM	±(PPM of Reading)		
		2 Years	90 Days	1 Year	2 Years
220V	10 Hz - 20 Hz	55	61	62	64
	20 Hz - 40 Hz	19	30	32	40
	40 Hz - 20 kHz	15	23	25	34
	20 kHz - 50 kHz	24	30	34	49
	50 kHz - 100 kHz		66	69	83
	100 kHz - 300 kHz		160	170	220
	300 kHz - 500 kHz		410	480	680
700V	10 Hz - 20 Hz	55	62	63	65
	20 Hz - 40 Hz	19	31	33	41
	40 Hz - 20 kHz	19	24	25	31
	20 kHz - 50 kHz		100	110	140
	50 kHz - 100 kHz		390	500	850
1000V	10 Hz - 20 Hz	55	62	63	65
	20 Hz - 40 Hz	19	31	33	41
	40 Hz - 20 kHz	19	24	25	31
	20 kHz - 50 kHz		100	110	140
	50 kHz - 100 kHz		390	500	850

Secondary Performance and Operating Characteristics

Voltage Range	Frequency Range	24 Hour AC Stability ±1°C Slow Filter Peak-Peak	Temperature Coefficient ¹		Input Resistance ²
			10°C to 40°C	0°C to 10°C 40°C to 50°C	
		±µV	PPM/°C		
2.2 mV	10 Hz - 20 Hz	0.4	50	50	>10 MΩ
	20 Hz - 40 Hz	0.4	50	50	
	40 Hz - 20 kHz	0.4	50	50	
	20 kHz - 50 kHz	0.4	50	50	
	50 kHz - 100 kHz	0.8	75	75	
	100 kHz - 300 kHz	1.5	100	100	
	300 kHz - 500 kHz	3.0	150	150	
500 kHz - 1 MHz	4.5	200	200		
7 mV	10 Hz - 20 Hz	0.4	15	15	>10 MΩ
	20 Hz - 40 Hz	0.4	15	15	
	40 Hz - 20 kHz	0.4	15	15	
	20 kHz - 50 kHz	0.4	15	15	
	50 kHz - 100 kHz	0.8	25	25	
	100 kHz - 300 kHz	1.5	60	60	
	300 kHz - 500 kHz	3.0	80	80	
500 kHz - 1 MHz	4.5	125	125		
22 mV	10 Hz - 20 Hz	0.4	5	5	>10 MΩ
	20 Hz - 40 Hz	0.4	5	5	
	40 Hz - 20 kHz	0.4	5	5	
	20 kHz - 50 kHz	0.4	5	5	
	50 kHz - 100 kHz	0.8	8	8	
	100 kHz - 300 kHz	1.5	10	10	
	300 kHz - 500 kHz	3.0	40	40	
500 kHz - 1 MHz	4.5	100	100		
		±(PPM of Reading)			
70 mV	10 Hz - 20 Hz	18	5	5	>10 MΩ
	20 Hz - 40 Hz	18	5	5	
	40 Hz - 20 kHz	18	5	5	
	20 kHz - 50 kHz	18	5	5	
	50 kHz - 100 kHz	24	8	8	
	100 kHz - 300 kHz	24	10	10	
	300 kHz - 500 kHz	48	30	30	
500 kHz - 1 MHz	150	75	75		
220 mV	10 Hz - 20 Hz	12	1.5	3.0	>10 MΩ
	20 Hz - 40 Hz	8	1.5	3.0	
	40 Hz - 20 kHz	8	1.5	3.0	
	20 kHz - 50 kHz	8	2.0	3.0	
	50 kHz - 100 kHz	18	5.0	8.0	
	100 kHz - 300 kHz	24	10.0	10.0	
	300 kHz - 500 kHz	36	20.0	20.0	
500 kHz - 1 MHz	120	50.0	50.0		

¹Add to uncertainty when more than 5°C from calibration temperature.

²Input capacitance approximately 100 pF.

Secondary Performance and Operating Characteristics (continued)

Voltage Range	Frequency Range	24 Hour AC Stability ±1 °C Slow Filter Peak-Peak	Temperature Coefficient ³		Input Resistance ⁴
			10 °C to 40 °C	0 °C to 10 °C 40 °C to 50 °C	
		±(PPM of Reading)	PPM/°C		
700 mV	10 Hz - 20 Hz	8	1.5	3.0	>10 MΩ
	20 Hz - 40 Hz	6	1.5	3.0	
	40 Hz - 20 kHz	6	1.5	3.0	
	20 kHz - 50 kHz	6	2.0	3.0	
	50 kHz - 100 kHz	12	5.0	8.0	
	100 kHz - 300 kHz	18	10.0	10.0	
	300 kHz - 500 kHz	36	20.0	20.0	
	500 kHz - 1 MHz	96	50.0	50.0	
2.2V	10 Hz - 20 Hz	8	1.5	3.0	>10 MΩ
	20 Hz - 40 Hz	5	1.5	3.0	
	40 Hz - 20 kHz	5	1.5	3.0	
	20 kHz - 50 kHz	5	2.0	3.0	
	50 kHz - 100 kHz	10	5.0	8.0	
	100 kHz - 300 kHz	18	10.0	10.0	
	300 kHz - 500 kHz	30	20.0	20.0	
	500 kHz - 1 MHz	90	50.0	50.0	
7V	10 Hz - 20 Hz	8	1.5	3.0	50 kΩ
	20 Hz - 40 Hz	5	1.5	3.0	
	40 Hz - 20 kHz	5	1.5	3.0	
	20 kHz - 50 kHz	5	2.0	3.0	
	50 kHz - 100 kHz	10	5.0	8.0	
	100 kHz - 300 kHz	18	15.0	15.0	
	300 kHz - 500 kHz	30	30.0	30.0	
	500 kHz - 1 MHz	90	65.0	65.0	
22V	10 Hz - 20 Hz	8	1.5	3.0	50 kΩ
	20 Hz - 40 Hz	5	1.5	3.0	
	40 Hz - 20 kHz	5	1.5	3.0	
	20 kHz - 50 kHz	5	2.0	3.0	
	50 kHz - 100 kHz	10	5.0	8.0	
	100 kHz - 300 kHz	18	15.0	15.0	
	300 kHz - 500 kHz	30	30.0	30.0	
	500 kHz - 1 MHz	90	65.0	65.0	
70V	10 Hz - 20 Hz	8	1.5	3.0	50 kΩ
	20 Hz - 40 Hz	5	1.5	3.0	
	40 Hz - 20 kHz	5	1.5	3.0	
	20 kHz - 50 kHz	5	2.0	3.0	
	50 kHz - 100 kHz	18	5.0	8.0	
	100 kHz - 300 kHz	36	15.0	15.0	
	300 kHz - 500 kHz	48	40.0	40.0	
	500 kHz - 1 MHz	120	75.0	75.0	
220V	10 Hz - 20 Hz	8	1.5	3.0	50 kΩ
	20 Hz - 40 Hz	5	1.5	3.0	
	40 Hz - 20 kHz	5	1.5	3.0	
	20 kHz - 50 kHz	5	2.0	3.0	
	50 kHz - 100 kHz	18	5.0	8.0	
	100 kHz - 300 kHz	36	15.0	15.0	
	300 kHz - 500 kHz	48	40.0	40.0	
700V	10 Hz - 20 Hz	8	1.5	4.0	500 kΩ
	20 Hz - 40 Hz	5	1.5	4.0	
	40 Hz - 20 kHz	5	1.5	4.0	
	20 kHz - 50 kHz	18	5.0	7.0	
	50 kHz - 100 kHz	36	15.0	15.0	
1000V	10 Hz - 20 Hz	8	1.5	4.0	500 kΩ
	20 Hz - 40 Hz	5	1.5	4.0	
	40 Hz - 20 kHz	5	1.5	4.0	
	20 kHz - 50 kHz	18	5.0	7.0	
	50 kHz - 100 kHz	36	15.0	15.0	

³Add to uncertainty when more than 5°C from calibration temperature.

⁴Input capacitance approximately 100 pF.

Secondary Performance and Operating Characteristics (continued)

Voltage Range	Aurorance Limits ⁵		Resolution	
	Upper	Lower	Filter Fast	Filter Med/Slow
2.2 mV	2.2 mV	600 μ V	0.1 μ V	0.1 μ V
7 mV	7 mV	1.9 mV	0.1 μ V	0.1 μ V
22 mV	22 mV	6 mV	0.1 μ V	0.1 μ V
70 mV	70 mV	19 mV	0.1 μ V	0.1 μ V
220 mV	220 mV	60 mV	0.1 μ V	0.1 μ V
700 mV	700 mV	190 mV	1.0 μ V	0.1 μ V
2.2V	2.2V	600 mV	1.0 μ V	0.1 μ V
7V	7V	1.9V	10 μ V	1.0 μ V
22V	22V	6V	10 μ V	1.0 μ V
70V	70V	19V	100 μ V	10 μ V
220V	220V	60V	100 μ V	10 μ V
700V	700V	190V	1.0 mV	100 μ V
1000V	1050V	600V	1.0 mV	100 μ V

⁵ In locked ranges readings may be made approximately 1% beyond the autorange limits.

Maximum non-destructive input:

1200V rms

Guard isolation: 10V peak

Volt-hertz product: 1×10^8

Frequency accuracy:

10-120 Hz: 100 ppm + 10 digits;

>120 Hz: 100 ppm + 2 digits over

0°C to 50°C

Frequency resolution:

1.00 Hz to 119.99 Hz

0.1200 kHz to 1.1999 kHz

1.200 kHz to 11.999 kHz

12.00 kHz to 119.99 kHz

0.1200 MHz to 1.1999 MHz

1.200 MHz to 11.999 MHz,

(wideband only)

12.00 MHz to 30.0 MHz,

(wideband only)

Reading rate:

<40 Hz: 2 seconds per reading

2 seconds at 40 Hz decreasing

linearly to 1 second at 200 Hz

>200 Hz: 1 second per reading

Maximum settling time to full specifications (in range lock):

Filter off:

1 sample

dc: 6 seconds

<200 Hz: 8 seconds

>200 Hz: 4 seconds

Filter fast:

4 averaged samples

dc: 10 seconds

<200 Hz: 16 seconds

>200 Hz: 8 seconds

Filter medium:

16 averaged samples

dc: 22 seconds

<200 Hz: 32 seconds

>200 Hz: 16 seconds

Filter slow:

32 averaged samples

dc: 40 seconds

<200 Hz: 64 seconds

>200 Hz: 32 seconds

Filter buffer restart limits:

Fine:

Fast: 10 counts

Medium/Slow:

<220 mV: 10 counts

>220 mV: 100 counts

Medium:

Fast: 100 counts

Medium/Slow:

<220 mV: 100 counts

>220 mV: 1000 counts

Course:

Fast: 1000 counts

Medium/Slow:

<220 mV: 1000 counts

>220 mV: 10000 counts

Input waveform: Specified for sinewave with THD less than 1%

Wideband Uncertainty Specifications (Option -03)

Voltage ⁶ Range	Frequency Range	Flatness ⁷ 1 Year ±3°C ±(% of Reading + μV)	Flatness ⁸ Temperature Coefficient PPM/°C	Absolute Uncertainty 0°C to 50°C ⁹ ±(% of Reading + μV)			Resolution
				90 Days	1 Year	2 Years	
2.2 mV	10 Hz - 30 Hz	0.10 + 0	75	0.5 + 1.2	0.6 + 1.5	0.8 + 2	0.1 μV
	30 Hz - 120 Hz	0.05 + 0	75	0.5 + 1.2	0.6 + 1.5	0.8 + 2	
	120 Hz - 1.2 kHz	0.05 + 0	75	0.5 + 1.2	0.6 + 1.5	0.8 + 2	
	1.2 kHz - 120 kHz	0.05 + 0	75	0.5 + 1.2	0.6 + 1.5	0.8 + 2	
	120 kHz - 500 kHz	0.07 + 1	75	0.5 + 1.2	0.6 + 1.5	0.8 + 2	
	500 kHz - 1.2 MHz	0.07 + 1	75				
	1.2 MHz - 2 MHz	0.07 + 1	100				
	2 MHz - 10 MHz	0.17 + 1	200				
	10 MHz - 20 MHz	0.30 + 1	200				
20 MHz - 30 MHz	0.70 + 2	400					
7 mV	10 Hz - 30 Hz	0.10 + 0	75	0.4 + 5	0.5 + 7	0.7 + 8	0.1 μV
	30 Hz - 120 Hz	0.05 + 0	75	0.4 + 5	0.5 + 7	0.7 + 8	
	120 Hz - 1.2 kHz	0.05 + 0	75	0.4 + 5	0.5 + 7	0.7 + 8	
	1.2 kHz - 120 kHz	0.05 + 0	75	0.4 + 5	0.5 + 7	0.7 + 8	
	120 kHz - 500 kHz	0.07 + 1	75	0.4 + 5	0.5 + 7	0.7 + 8	
	500 kHz - 1.2 MHz	0.07 + 1	75				
	1.2 MHz - 2 MHz	0.07 + 1	100				
	2 MHz - 10 MHz	0.10 + 1	200				
	10 MHz - 20 MHz	0.17 + 1	200				
20 MHz - 30 MHz	0.37 + 1	300					
		±(% of Reading)					
22 mV	10 Hz - 30 Hz	0.10	75	0.4 + 10	0.5 + 13	0.7 + 16	0.1 μV
	30 Hz - 120 Hz	0.05	75	0.4 + 10	0.5 + 13	0.7 + 16	
	120 Hz - 1.2 kHz	0.05	75	0.4 + 10	0.5 + 13	0.7 + 16	
	1.2 kHz - 120 kHz	0.05	75	0.4 + 10	0.5 + 13	0.7 + 16	
	120 kHz - 500 kHz	0.07	75	0.4 + 10	0.5 + 13	0.7 + 16	
	500 kHz - 1.2 MHz	0.07	75				
	1.2 MHz - 2 MHz	0.07	75				
	2 MHz - 10 MHz	0.10	100				
	10 MHz - 20 MHz	0.17	100				
20 MHz - 30 MHz	0.37	200					
70 mV	10 Hz - 30 Hz	0.10	40	0.4 + 20	0.5 + 30	0.6 + 40	1.0 μV
	30 Hz - 120 Hz	0.05	40	0.4 + 20	0.5 + 30	0.6 + 40	
	120 Hz - 1.2 kHz	0.05	40	0.4 + 20	0.5 + 30	0.6 + 40	
	1.2 kHz - 120 kHz	0.05	40	0.4 + 20	0.5 + 30	0.6 + 40	
	120 kHz - 500 kHz	0.05	40	0.4 + 20	0.5 + 30	0.6 + 40	
	500 kHz - 1.2 MHz	0.05	40				
	1.2 MHz - 2 MHz	0.05	75				
	2 MHz - 10 MHz	0.10	100				
	10 MHz - 20 MHz	0.15	100				
20 MHz - 30 MHz	0.35	200					
220 mV	10 Hz - 30 Hz	0.10	40	0.3 + 60	0.4 + 80	0.5 + 100	1.0 μV
	30 Hz - 120 Hz	0.04	40	0.3 + 60	0.4 + 80	0.5 + 100	
	120 Hz - 1.2 kHz	0.04	40	0.3 + 60	0.4 + 80	0.5 + 100	
	1.2 kHz - 120 kHz	0.04	40	0.3 + 60	0.4 + 80	0.5 + 100	
	120 kHz - 500 kHz	0.04	40	0.3 + 60	0.4 + 80	0.5 + 100	
	500 kHz - 1.2 MHz	0.05	40				
	1.2 MHz - 2 MHz	0.05	75				
	2 MHz - 10 MHz	0.10	100				
	10 MHz - 20 MHz	0.15	100				
20 MHz - 30 MHz	0.35	200					
700 mV	10 Hz - 30 Hz	0.10	40	0.3 + 200	0.4 + 300	0.5 + 400	10.0 μV
	30 Hz - 120 Hz	0.03	40	0.3 + 200	0.4 + 300	0.5 + 400	
	120 Hz - 1.2 kHz	0.03	40	0.3 + 200	0.4 + 300	0.5 + 400	
	1.2 kHz - 120 kHz	0.03	40	0.3 + 200	0.4 + 300	0.5 + 400	
	120 kHz - 500 kHz	0.03	40	0.3 + 200	0.4 + 300	0.5 + 400	
	500 kHz - 1.2 MHz	0.05	40				
	1.2 MHz - 2 MHz	0.05	75				
	2 MHz - 10 MHz	0.10	100				
	10 MHz - 20 MHz	0.15	100				
20 MHz - 30 MHz	0.35	200					

⁶ Range limits same as INPUT1 or INPUT2.

⁷ Relative 1 kHz.

⁸ Add to flatness specifications when more than 3°C from calibration temperature.

⁹ At input connector.

Maximum non-destructive input: 200V rms

Wideband guard isolation: 0.5V peak

Wideband input impedance:

1 kHz: 50Ω (±0.5%)

30 MHz: 50Ω (±5%)

Wideband VSWR with 50Ω source:

1 kHz: 1.005

30 MHz: 1.05

Wideband Uncertainty Specifications (Option -03) (continued)

Voltage ¹⁰ Range	Frequency Range	Flatness ¹¹ 1 Year ±3°C ±(% of Reading)	Flatness ¹² Temperature Coefficient PPM/°C	Absolute Uncertainty 0°C to 50°C ¹³ ±(% of Reading + μV)			Resolution
				90 Days	1 Year	2 Years	
2.2V	10 Hz - 30 Hz	0.10	40	0.3 + 300	0.35 + 400	0.4 + 500	10.0 μV
	30 Hz - 120 Hz	0.03	40	0.3 + 300	0.35 + 400	0.4 + 500	
	120 Hz - 1.2 kHz	0.03	40	0.3 + 300	0.35 + 400	0.4 + 500	
	1.2 kHz - 120 kHz	0.03	40	0.3 + 300	0.35 + 400	0.4 + 500	
	120 kHz - 500 kHz	0.03	40	0.3 + 300	0.35 + 400	0.4 + 500	
	500 kHz - 1.2 MHz	0.05	40				
	1.2 MHz - 2 MHz	0.05	75				
	2 MHz - 10 MHz	0.10	100				
	10 MHz - 20 MHz	0.15	100				
	20 MHz - 30 MHz	0.35	200				
7V	10 Hz - 30 Hz	0.10	40	0.3 + 500	0.35 + 800	0.4 + 1000	100.0 μV
	30 Hz - 120 Hz	0.03	40	0.3 + 500	0.35 + 800	0.4 + 1000	
	120 Hz - 1.2 kHz	0.03	40	0.3 + 500	0.35 + 800	0.4 + 1000	
	1.2 kHz - 120 kHz	0.03	40	0.3 + 500	0.35 + 800	0.4 + 1000	
	120 kHz - 500 kHz	0.03	40	0.3 + 500	0.35 + 800	0.4 + 1000	
	500 kHz - 1.2 MHz	0.05	40				
	1.2 MHz - 2 MHz	0.05	75				
	2 MHz - 10 MHz	0.10	100				
	10 MHz - 20 MHz	0.15	100				
	20 MHz - 30 MHz	0.35	200				

¹⁰ Range limits same as INPUT1 or INPUT2.

¹¹ Relative 1 kHz.

¹² Add to flatness specifications when more than 3°C from calibration temperature.

¹³ At input connector.

Shunt input characteristics

The shunt input was designed to allow ac/dc current transfers using the Fluke A40 Series Current Shunts. 5790A-7001 A40/A40A Current Shunt Adapter and Cable required.

Shunt model	Current range
A40	2.5 mA-5A
A40A	5A-20A

Input resistance: 91Ω ± 1%

Operating input voltage: 250 mV to 500 mV

Maximum non-destructive input: 50V rms

EMI/RFI: Complies with FCC Part 15 Subpart B, Class B; EN50081-1, EN50082-1

Size:

Height: 17.8 cm (7 in) standard rackmount + 1.5 cm (0.6 in)

Width: 43.2 cm (17 in)

Depth: 63 cm (24.8 in)

Maximum power:

5790A: 95 VA

With wideband: 120 VA

Weight:

5790A: 24 kg (53 lb)

With wideband: 24.5 kg (54 lb)

Line power: 47 Hz to 63 Hz; ± 10% of selectable line voltages: 100V, 110V, 115V, 120V, 200V, 220V, 230V, 240V

Safety: Designed to comply with UL3111; EN61010; CSA C22.2 No. 1010; ANSI/ISI S82.01-1994

Remote interfaces: RS-232, IEEE-488

General specifications

Warm-up time: 30 minutes

Relative humidity:

Operating: 45% to 50°C

75% to 45°C

95% to 30°C

Storage: <95% non-condensing

Altitude:

Operating: 3,050m (10,000 ft)


Non-operating: 12,200m (40,000 ft)

Temperature:

Operating: 0°C to 50°C

Calibration: 15°C to 35°C

Storage: -40°C to 70°C

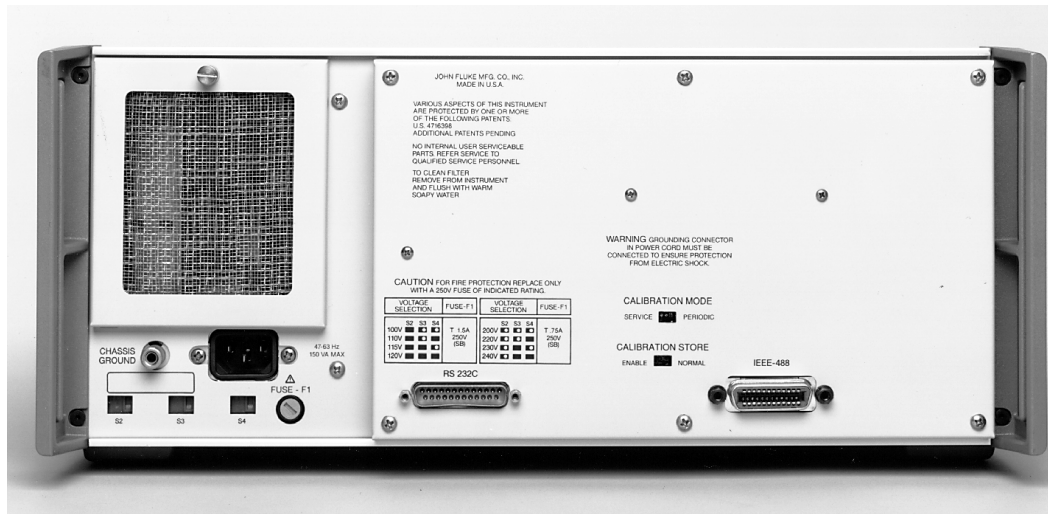

5790A rear panel.

Ordering Information

Model

5790A AC Measurement Standard

Options

5790A-03 Wideband AC Measurement

Accessories

5440A-7002 Low Thermal Cable Set

792A-7003 Transfer Switch

792A-7004 A40 Current Shunt Adapter.

Connects directly to Type-N input connector to permit use with A40 Current Shunts. Not compatible with A40A Current Shunts.

5790A-7001 A40/A40A Current Shunt Adapter and Cable. Connects to current shunt binding posts to permit use with both A40 and A40A Current Shunts.

A40 Current Shunts (10, 20, 50, 100, 200, 300, 500 mA and 1, 2, 3, 5A). Requires 792A-7004 or 5790A-7001.

A40A Current Shunts (10 and 20A). Requires 5790A-7001.

Y5737 5790A Rackmount Kit. Includes 24" slides that allow for side ventilation.

Y8021 Shielded IEEE-488 Cable, 1m

Y8022 Shielded IEEE-488 Cable, 2m

Y8023 Shielded IEEE-488 Cable, 4m



Fluke. *Keeping your world up and running.*

Fluke Corporation

PO Box 9090, Everett, WA USA 98206

Fluke Europe B.V.
PO Box 1186, 5602 BD
Eindhoven, The Netherlands

For more information call:
In the U.S.A. (800) 443-5853 or
Fax (425) 356-5116
In Europe (31 40) 2 678 200 or
Fax (31 40) 2 678 222
In Canada (905) 890-7600 or
Fax (905) 890-6866

From other countries (425) 356-5500
Web access: <http://www.fluke.com>

© 1996 Fluke Corporation. All rights reserved.
Printed in U.S.A. 9/96 AO415UEN Rev D

Printed on recycled paper.